


CLEARVIEW®

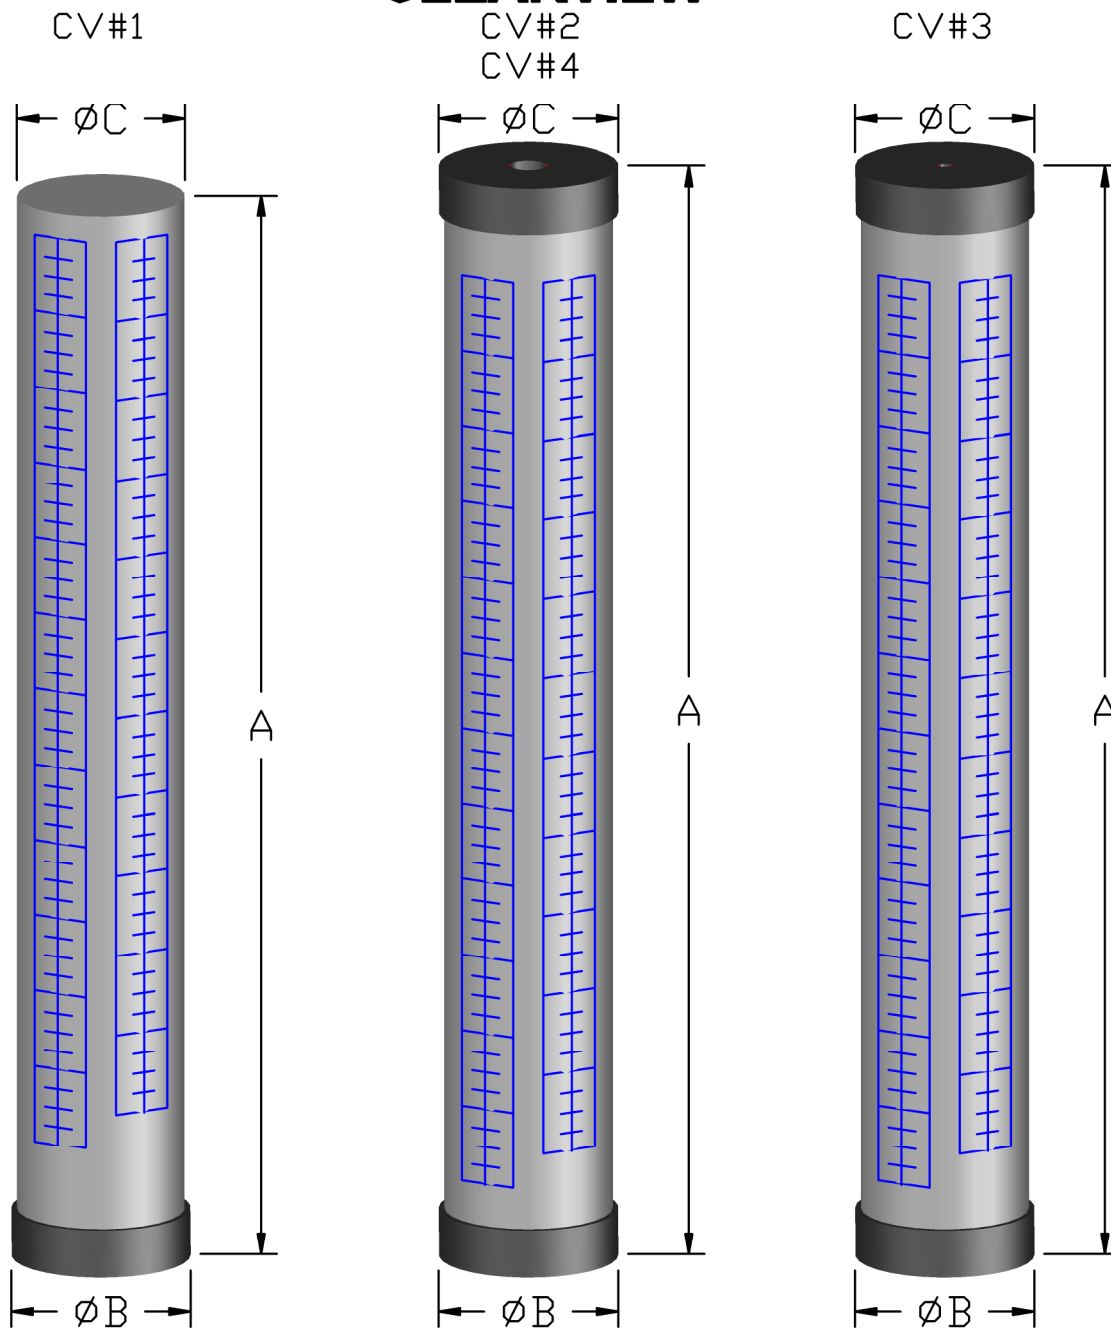

MODEL	SIZE ml(GPH)	DIV ml(GPH)	A (in.)	ØB (in.)	ØC (in.)	Connection	Top Conn.
CV#1	100 (1.60)	1.0 (0.02)	10.13	1.4	1.1	1/2' (DN 15)	OPEN
	250 (4.00)	2.0 (0.05)	10.88	1.9	1.6		
	500 (8.00)	5.0 (0.05)	12.13	2.4	2.1		
	1000 (16.0)	10.0 (0.125)	16.13	2.8	2.5	1' (DN 25)	
	2000 (32.0)	20.0 (0.25)	20.00	3.5	3.1		
	4000 (64.0)	25.0 (0.25)	22.00	4.5	4.1	2' (DN 50)	
	10000 (160)	200.0 (2.00)	22.50	6.9	6.5		
	15000 (240)	200.0 (2.00)	32.50	6.9	6.5		
20000 (320)	200.0 (2.00)	42.50	6.9	6.5			
CV#2 & CV#4	100 (1.60)	1.0 (0.02)	10.50	1.4	1.4	1/2' (DN 15)	1/2' (DN 15)
	250 (4.00)	2.0 (0.05)	11.25	1.9	1.9		
	500 (8.00)	5.0 (0.05)	12.50	2.4	2.4		
	1000 (16.0)	10.0 (0.125)	16.50	2.8	2.8	1' (DN 25)	
	2000 (32.0)	20.0 (0.25)	20.50	3.5	3.5		
	4000 (64.0)	25.0 (0.25)	22.50	4.5	4.5	2' (DN 50)	
	10000 (160)	200.0 (2.00)	23.00	6.9	6.9		
	15000 (240)	200.0 (2.00)	33.00	6.9	6.9		
20000 (320)	200.0 (2.00)	43.00	6.9	6.9			
CV#3	100 (1.60)	1.0 (0.02)	10.50	1.4	1.4	1/2' (DN 15)	DUST CAP
	250 (4.00)	2.0 (0.05)	11.25	1.9	1.9		
	500 (8.00)	5.0 (0.05)	12.50	2.4	2.4		
	1000 (16.0)	10.0 (0.125)	16.50	2.8	2.8	1' (DN 25)	
	2000 (32.0)	20.0 (0.25)	20.50	3.5	3.5		
	4000 (64.0)	25.0 (0.25)	22.50	4.5	4.5	2' (DN 50)	
	10000 (160)	200.0 (2.00)	23.00	6.9	6.9		
	15000 (240)	200.0 (2.00)	33.00	6.9	6.9		
20000 (320)	200.0 (2.00)	43.00	6.9	6.9			

NOTE:
CV#4 CALIBRATION CYLINDERS HAVE
REMOVABLE TOP CAPS.

DO NOT COPY WITHOUT PRIOR WRITTEN APPROVAL FROM PRIMARY FLUID SYSTEMS INC.

PRIMARY FLUID SYSTEMS INC.

1050 Cooke Blvd., Burlington, Ontario L7T 4A8

CLEARVIEW CV-SERIES
CALIBRATION CYLINDERS (PVC)

DATE ISSUED: JULY-29-2014 | SCALE: NTS | SHEET: 1 OF 1

TOLERANCE: +/- 0.25" | DRAWN BY: NEAL YOON

APPROVED BY: DWG NO.: ADV_CV_CALCYL1 REV.# 4